

Snowmass 2001

July 16, 2001

# **Calorimeter for JLC Experiment**

Hiroyuki Matsunaga  
University of Tsukuba

JLC-CAL group is a collaboration of  
Kobe, Konan, Shinshu, Tsukuba, and KEK

# 1) Required Performance

Design Criteria in a de-coupled CAL parameter space

**2-jet mass resolution** better than  $Z$ ,  $W$

- **Hardware Compensation** for excellent hadron energy **Resolution and Linearity**
- **Fine Granularity** for precise topological reconstruction


No software compensation

No extremely-fine granularity

## Technology Choice

### **Tile/Fiber Sampling Calorimeter**

- Crackless Hermeticity
- Low Cost
- Design Flexibility
- Well-established technology

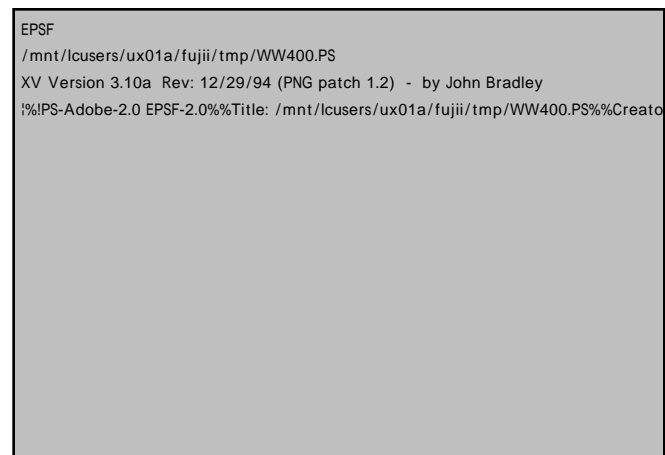

Reconstructed W mass for e+e- -> W+W- at S=400GeV


Result of quick-simulation. SHmax is not used for analysis.

Thus contribution of track-cluster association error is as

large as  $\sim 1.9\text{GeV}$ . Better result expected with SHmax analysis.

## 2) Basic parameters of revised baseline JLC calorimeter

magnetic-field option	2T-case	3T-case
Inner Radius	250cm	160cm
Outer Radius	400cm	340cm
Angular Coverage	$ \cos  < 0.985$	$ \cos  < 0.966$ (Full)
	$ \cos  < 0.994$	$ \cos  < 0.991$ (Partial)
<b>SHmax scheme</b>	<b>Scintillator-Strip Array</b> ( 1cm-wide )	option=Si-pad (1cm x 1cm)
<b>EMC</b>	$\sigma_E/E = 15\%/\sqrt{E} + 1\%$	
transverse	<b>6cm x 6cm</b> (24mrad)	<b>4cm x 4cm</b> (24mrad)
longitudinal	3 sections (6+12+20 layers)	
<b>HCAL</b>	$\sigma_E/E = 40\%/\sqrt{E} + 2\%$	
transverse	<b>18cm x 18cm</b> ( 72mrad )	<b>12cm x 12cm</b> ( 72mrad )
longitudinal	4 sections (25+30+35+40 layers)	
Thickness		
<b>PreSH</b>	<b>4Xo ( 4mm x 6 layers )</b>	
<b>EMC</b>	<b>23Xo ( 4mm x 22 layers )</b>	
<b>HCAL</b>	<b>6.5λo ( 8mm x 130 layers )</b>	

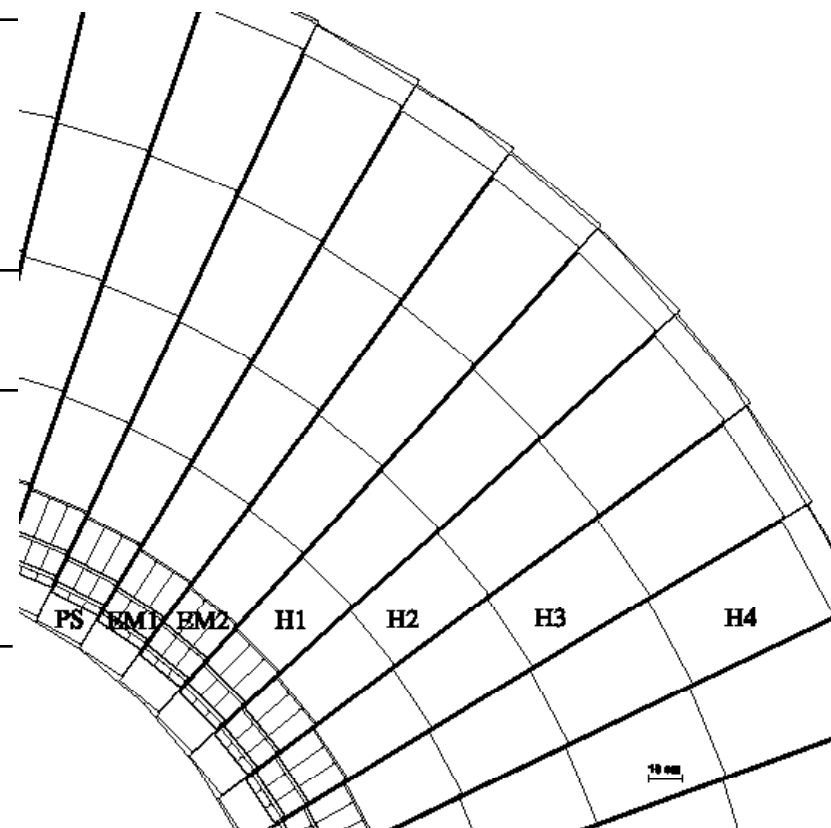

Configuration of Baseline Barrel Calorimeter

### 3) Proof of Performance

#### [A] Energy Resolution & Linearity

- Related to Material Choice and Global Design
- Must be verified by **Beam Test**

#### [B] Granularity


- Related to Component Design
  - Must be verified by **Full Simulation**
- ..... Easy to tune at any stage in the case of Tile/Fiber scheme

#### Strategy;

- **1st** Establish energy resolution & linearity with tile/fiber test module  
**DONE**
- **2nd** Optimize granularity by full simulation with tile/fiber structure implemented  
**In Progress**

**[A] Beam tests done at KEK (1-4GeV) and at FNAL (10-200GeV) to prove ;**

- a) **Energy Resolution** / Gaussian Response / Hardware Compensation
- b) **Linearity** / Dynamic Range
- c) **Tower Boundary Uniformity**
- d) **e/ separation** capability

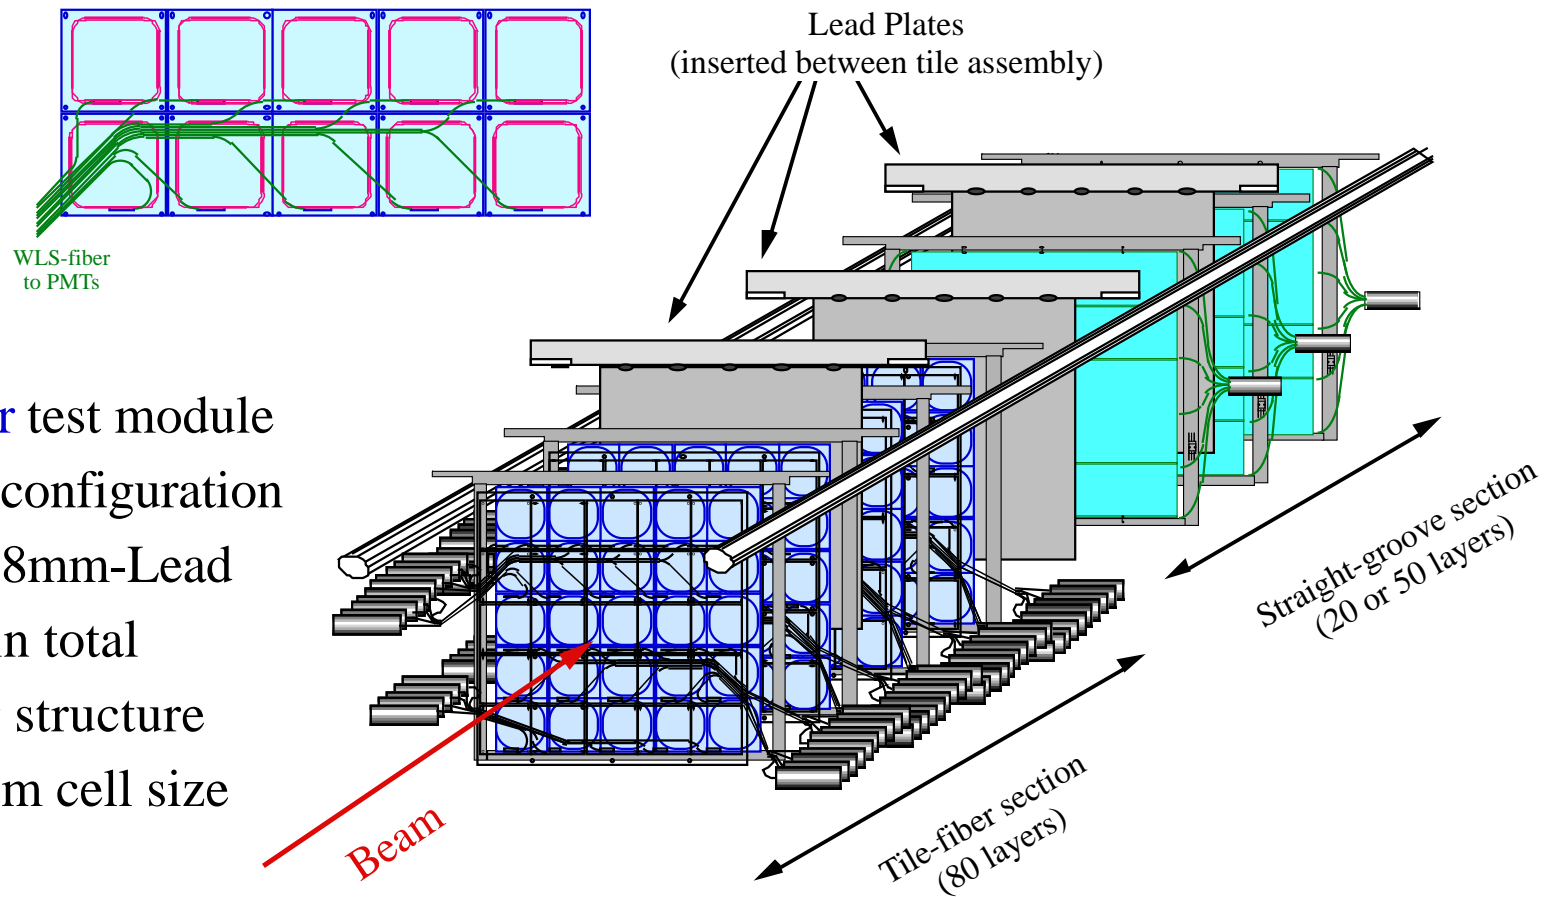

Schematic View of  
**Hadron Calorimeter** test module  
with **Tile/Fiber** configuration

- 2mm-Sci + 8mm-Lead
- 130 layers in total
- 5 x 5 tower structure
- 20cm x 20cm cell size

## a) Energy Resolution

EPSF  
(resolution.eps)  
Adobe Illustrator(R) 8.0  
(2/3/01) (5:08 PM)

$\pi$  ;  $\sigma_E/E = 46.7 \pm 0.6\%/\sqrt{E} + 0.9 \pm 0.9\%$   
worse than design due to 'fiber-routing' acryl plate


Effect of acryl plate (measured by beam tests)

- No effect on compensation
  - if placed downstream of scintillator
- No effect on EM energy resolution regardless its location
- Deteriorate hadron energy resolution regardless its location

Measured energy resolution of tile/fiber  
hadron calorimeter test module





## b) Linearity

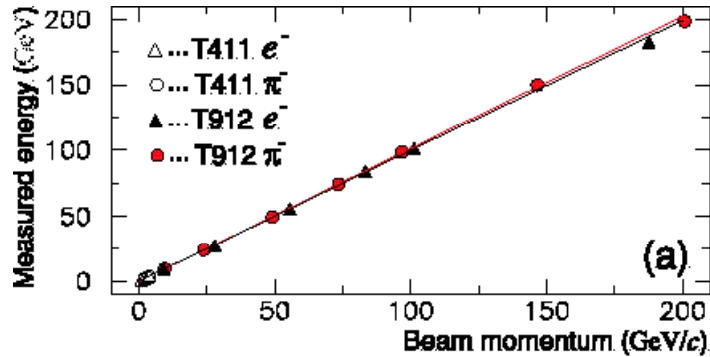

Nice Linearity thanks to Hardware Compensation.  
( better than 1% from 2 GeV to 150 GeV )



## c) Tower Boundary Response

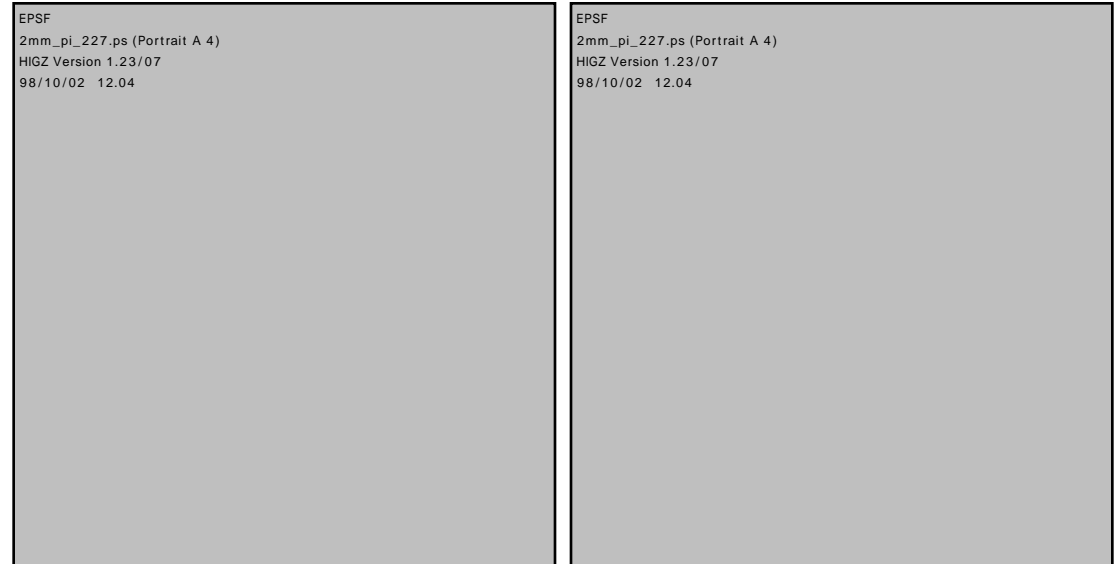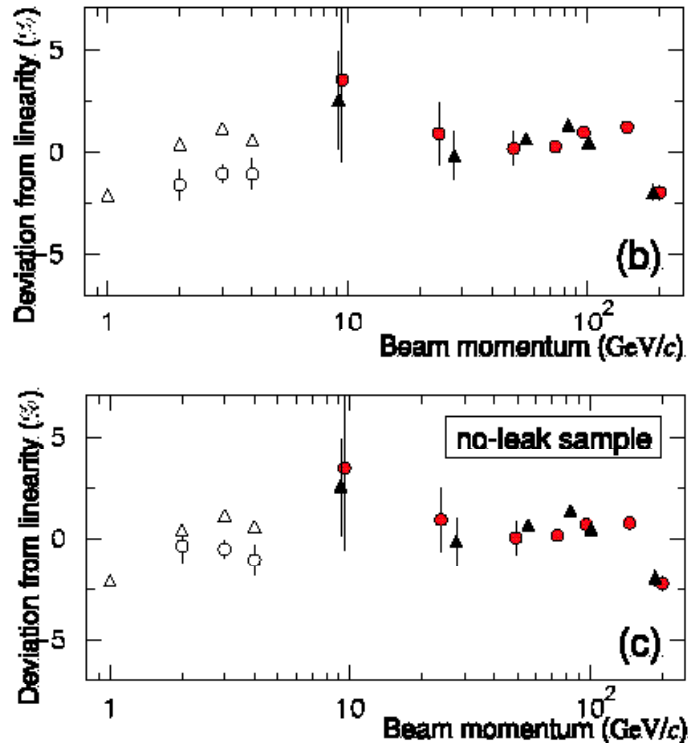

- No significant anomaly was observed at the tower boundary for pions.
- Slight anomaly was observed for electrons.

EM module must be designed with more uniform response.

## d) $e^-$ separation and PreSH/SHmax

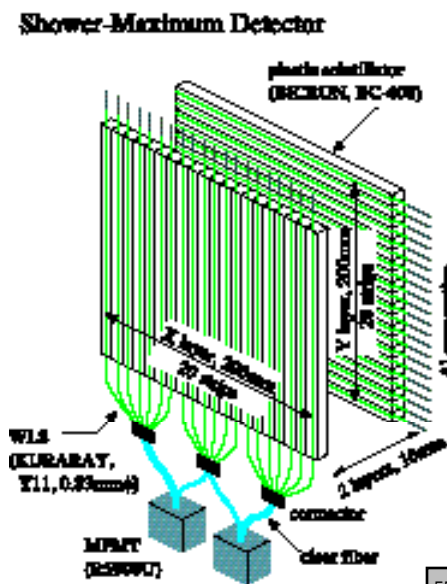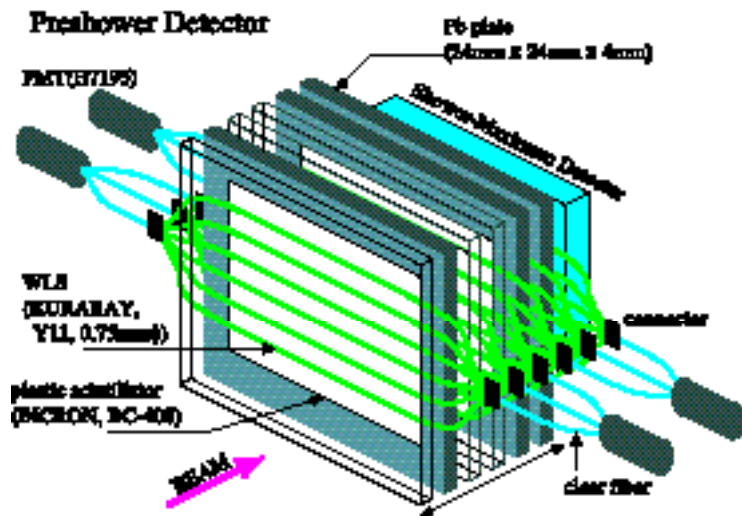

Combined performance of

- PreSH
- SHmax (Scint-Strip)
- HCAL

measured with test beam.

- pion rejection  $\sim 1/1400$
- with  $\epsilon \sim 98\%$
- **Quite Satisfactory**
- position resolution 2~3mm  
due to noise/cross talk  
Needs improvements

EPSF  
ps/pre\_spr.eps  
HIGZ Version 1.23/09  
00/02/05 16.48



## [B] Granularity Optimization

### Optimization with a full simulator based on GEANT3


- Tuning of calorimeter response in progress
- Hadron-clustering algorithm under development
- Cluster-track association algorithm under development

- Implementation of hadron shower generator **with realistic fluctuation**  
Still working hard to make 'Un-Correlated' distribution function.

**Yet a lot to do before reconstruction of physics processes for optimization.**



Un-correlated fluctuation for EM

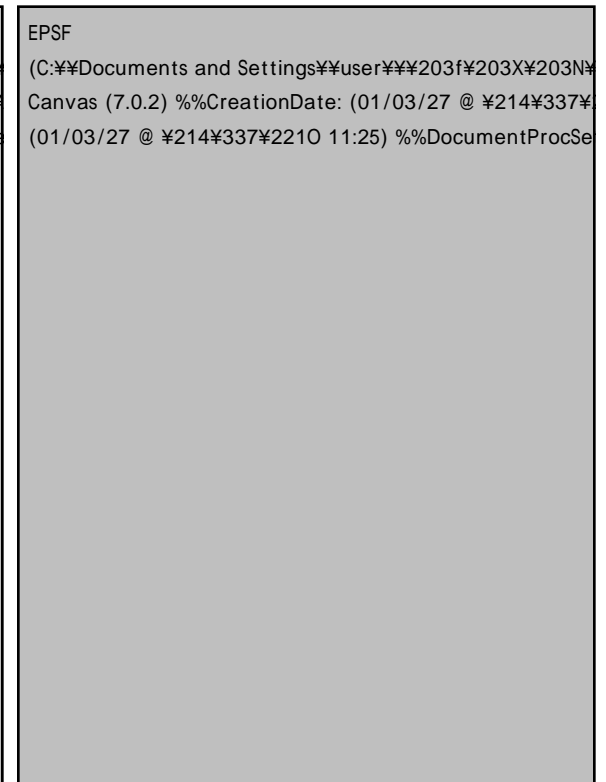


Correlated fluctuation for hadrons

## 4) Other R&D Items

### a) Scintillator-strip EMCAL

- much finer-granularity
- reasonable cost by **casting/extrusion** of strips
- non-uniformity over a strip  $\sim 4.8\%$   
similar to traditional square tiles ( $\sim 4.6\%$  )
- requires **super multi-channel photo-detectors**
- **crossed-strip** layout need study  
**ghost-rejection** capability by full simulation
- energy decomposition algorithm be studied  
for multi-hit in a cell.



Photon yield uniformity over a 1cm-wide strip

## b) Photon Detectors

- EMC/HCAL


multi-channel HPD/HAPD : promising (however cost-down needed)

- Scintillator-Strip EMC/SHmax need


super-multichannel photo-detector.

- 61ch-HPD ; tests in progress

- **EBCCD** ; tests in progress. **Higer gain needed.**

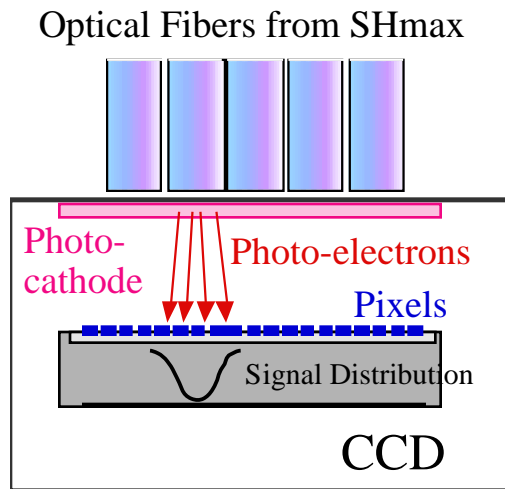

Principle of EBCCD

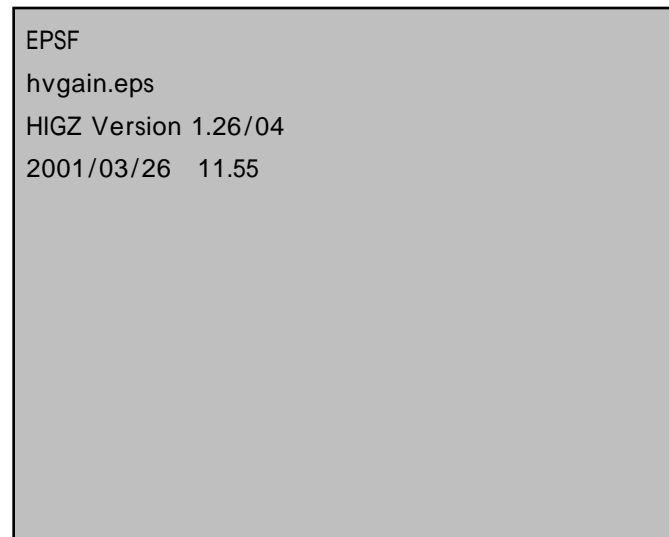

Gain vs photo-cathode voltage for proximity-focused EBCCD

## C) Strong Lead Alloy

Hardware Compensation ... Lead as passive/structural material

==> Lead alloy with high rigidity and tensile strength needed.

Temporary target = strength of copper

	tensile strength (yield)
<b>Copper</b>	<b>64MPa</b>
Pure Lead	7MPa
<b>Lead Alloy</b>	<b>50MPa</b> (preliminary)

- Other samples being tested.
- Young modulus under calibration.

EPSF  
(Pb1052-1.xls)  
(Microsoft Excel: AdobePS 8.5.2)  
(17:33 2001¥224N 7¥214¥216 5¥223¥372 ¥226¥330¥227j¥223¥372)

## 5) Summary

Baseline design of JLC calorimeter

- high performance expected ; **hermeticity, resolution, linearity**
- with **well-established technology** ; tile/fiber scheme
- with **reasonable cost** ; casting enables further cost reduction
- **design flexibility** ; completely decoupled resolution & granularity  
by hardware compensation scheme

However verification with full simulation is severely behind schedule.